




MG1 (nom 125V)	
V	I (ua)
10	0.2
20	0.3
30	0.3
40	0.4
50	0.4
60	0.5
70	0.6
80	0.6
90	0.6
100	0.8
110	1.1
120	1.2
130	1.3
140	1.5
150	1.7
160	1.8

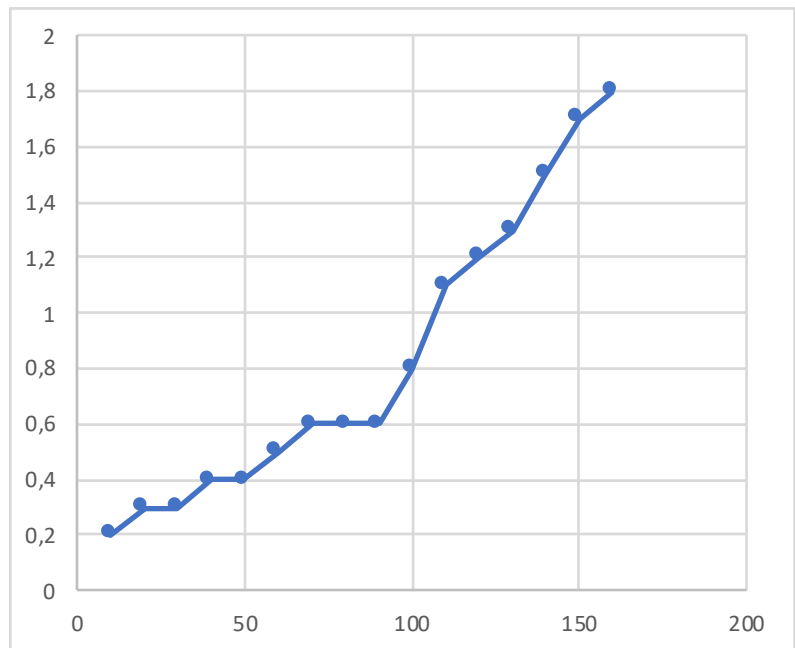


MG3 (nom 135V)	
V	I (ua)
10	0.1
20	0.2
30	0.2
40	0.2
50	0.2
60	0.2
70	0.2
80	0.2
90	0.3
100	0.3
110	0.3
120	0.4
130	0.4
140	0.5
150	0.6
160	0.8
170	1
180	1.3

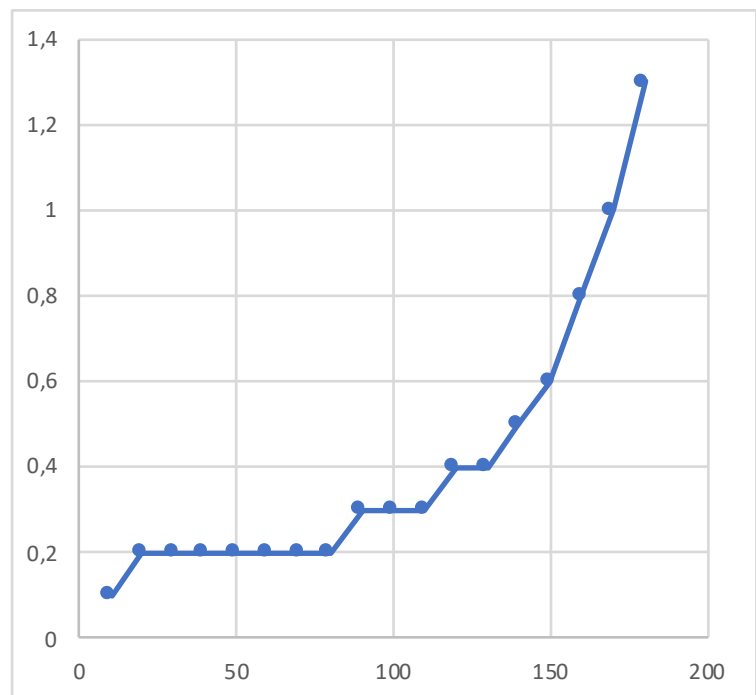


MG4 (nom 95V)	
V	I (ua)
10	0
20	0
30	0
40	0
50	0
60	0.1
70	0.3
80	0.6
90	0.9
100	1.6

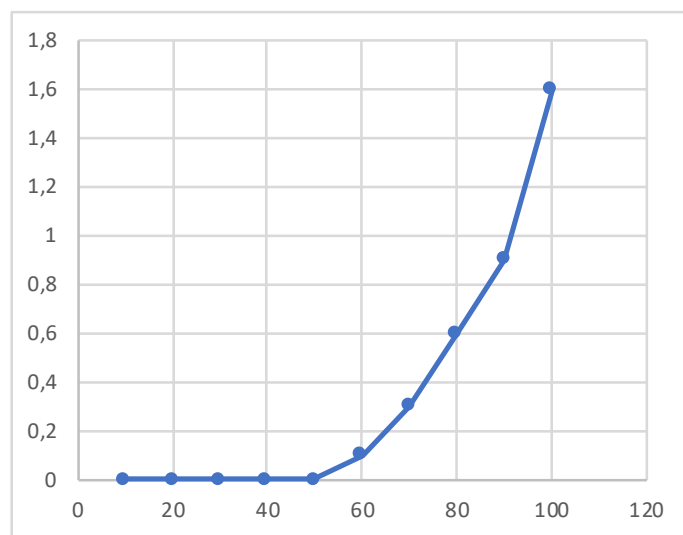


MG5 (nom 140V)	
V	I (ua)
10	0
20	0
30	0
40	0
50	0
60	0
70	0
80	0.1
90	0.1
100	0.1
110	0.2
120	0.3
130	0.5
140	0.9
150	1.4
160	2

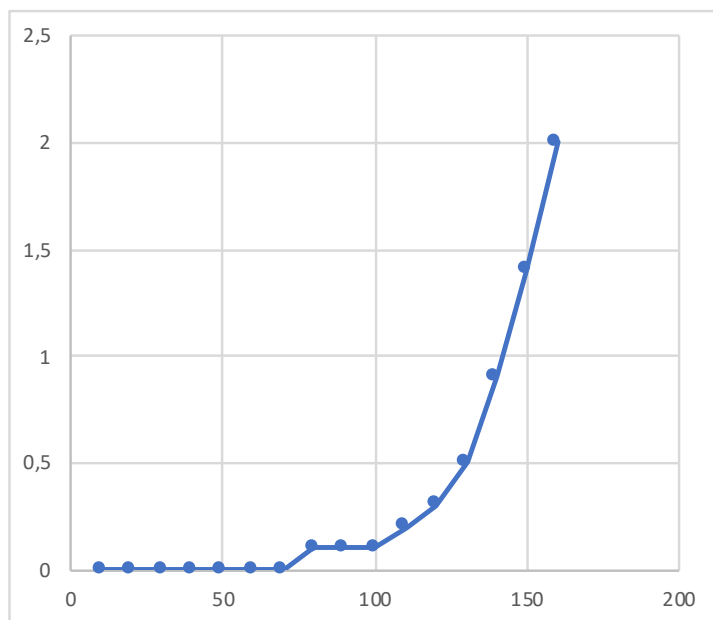

MG7 (nom 125V)	
V	I (ua)
10	0.1
20	0.2
30	0.2
40	0.2
50	0.2
60	0.3
70	0.3
80	0.4
90	0.4
100	0.5
110	0.9
120	1.8

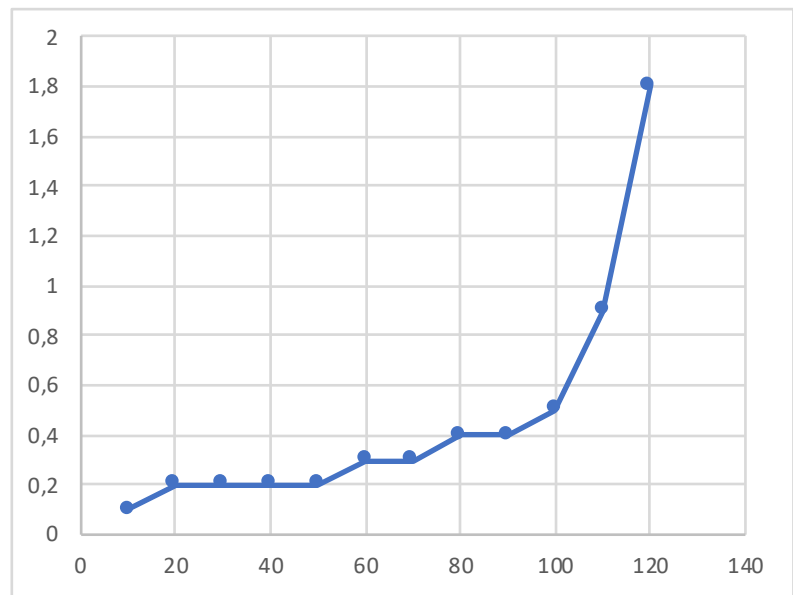

MG11 (nom ??V)	
V	I (ua)
10	0.2
20	0.4
30	0.5
40	0.5
50	0.6
60	0.6
70	0.6
80	0.6

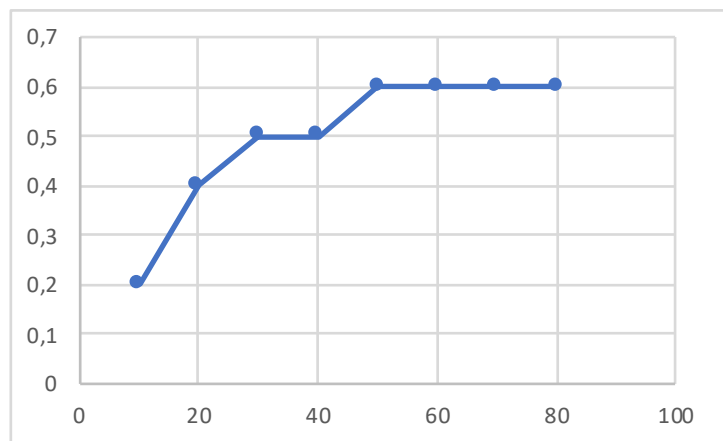

Detectors seems to respond accordingly with the previous measurements from Marlène. Annular detector curve is quite strange...